

USAGE GUIDELINES FOR SWIFT SLIDER AND SWIFT ULTRASLIDE SYSTEM






BREATHABLE PATIENT REPOSITIONER



STEP 1

Place Swift Slider on bottom sheet with blue, low-friction taffeta panel down.


Note: Ensure brakes of bed are on.

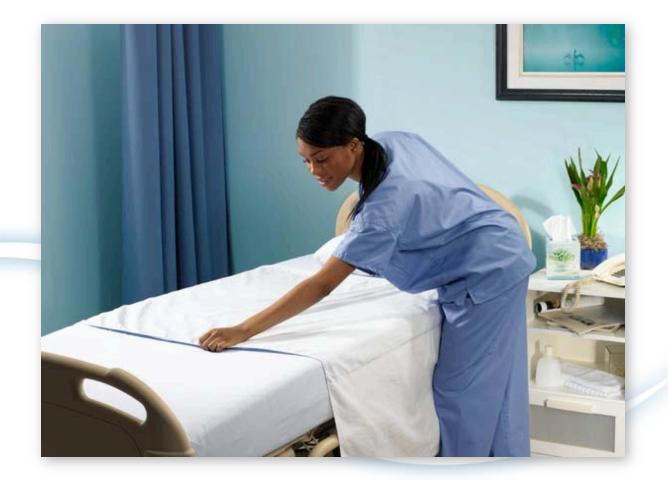



STEP 2a


Tuck in flaps, once Swift Slider has been placed.

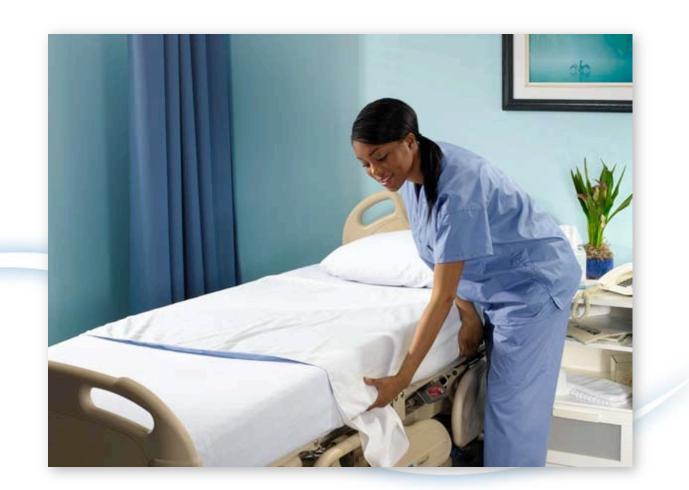



STEP 2b

Place incontinence pad on top of Swift Slider (if needed).

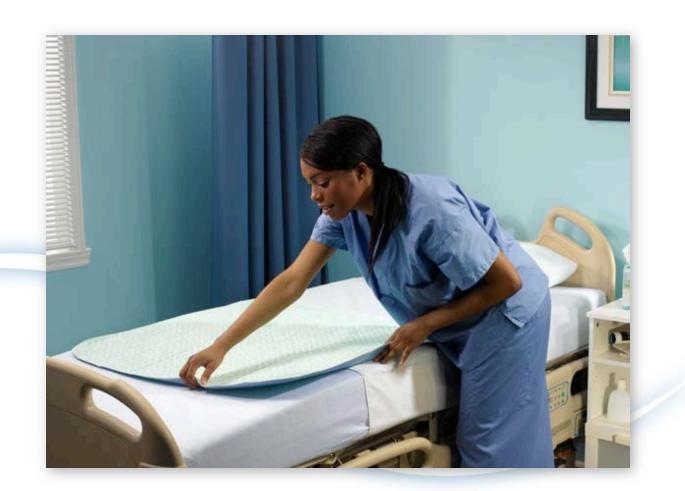



STEP 3

Position patient centrally on white Swift Slider surface. The central panel should support patient from the neck to just below the buttocks.

Note: Place pillow at head of bed to avoid accidental head injury.





STEP 4

Ensure there is a caregiver on each side of bed.

Note: When possible, bed height should be at caregivers' upper thigh level.





STEP 5

Un-tuck flaps.





STEP 6

Bend patient's knees to protect heels from being dragged across linens.





STEP 7

Hold Swift Slider with two hands - One at shoulder height and one at hip height.

To move patient, gather Swift Slider as close as possible to patient's body. Reposition by laterally shifting body weight.





STEP 7

Alternate repositioning method: Rabbit Ears technique





STEP 8

Once patient has been repositioned, smooth out Swift Slider and tuck flaps securely under mattress.





Note: If the head of the bed needs to be elevated, raise the knee gatch to prevent the patient from sliding down the mattress.

Position the patient's hips in the bend of the bed. If hips go above that zone, patient will slide down by force of gravity.

Please remember:

We strongly advise against using Swift Slider for lifting.









STEP 1

Place UltraSlide bottom sheet over the mattress, as you would a normal fitted sheet.


Note: Ensure brakes of bed are on.





STEP 2

Place Swift Slider across UltraSlide bottom sheet, with blue sides facing each other.

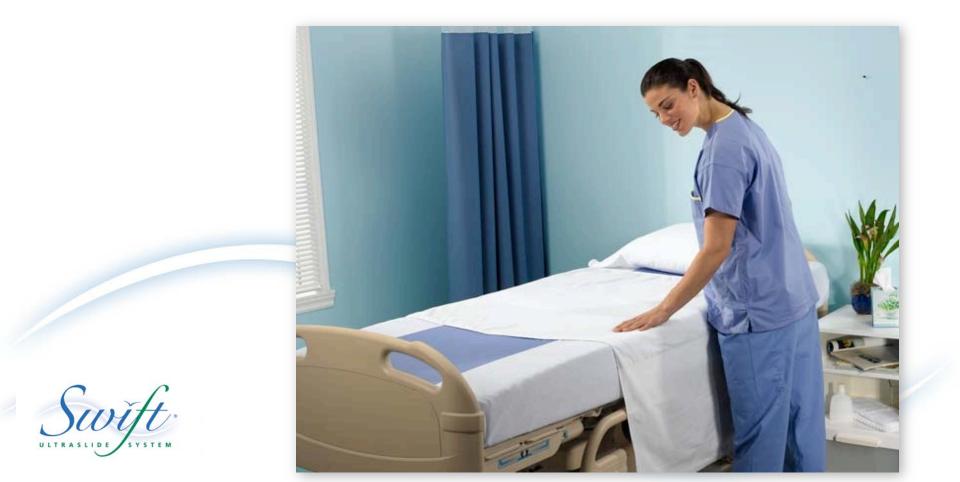

STEP 3

Tuck in flaps, once Swift Slider has been placed.

Note: Place incontinence pad on top of Swift Slider (if needed).





STEP 4

Position patient centrally on white Swift Slider surface. The central panel should support patient from the neck to just below the buttocks.

Note: Place pillow at head of bed to avoid accidental head injury.





STEP 5

Reposition patient using appropriate protocol.

Refer to usage guidelines for Swift Slider - Steps 4 through 7.



STEP 6

Once patient has been repositioned, smooth out Swift Slider and tuck flaps securely under mattress.





Note: If the head of the bed needs to be elevated, raise the knee gatch to prevent the patient from sliding down the mattress.

Position the patient's hips in the bend of the bed. If hips go above that zone, patient will slide down by force of gravity.

Please remember:

We strongly advise against using Swift Slider for lifting.







MOVING IN THE RIGHT DIRECTION

www.mipinc.com

Toll free: 800-361-4964

